

IBD-SCAN®

An ELISA for the Quantitative Measurement of Fecal Lactoferrin,
a Marker of Fecal Leukocytes, and when Elevated,
an Indicator of Intestinal Inflammation
Catalog No. T5009 (96 Tests)

Distributed by



NL Charles Stulemeijerweg 15, 5026 RS Tilburg
T 013 467 27 00 F 013 467 80 16
B Rond Point Schuman 6, 1040 Brussels
T 02 280 05 06 F 02 280 06 61
orange@orangemedical.nl www.orangemedical.nl

Developed and Manufactured by



TECHLAB®




U. S. Patent # 7,192,724


Australian Patent # 2002220029

International Symbol Key:

 Catalog Number

 *In Vitro* Diagnostic Medical Device


 Lot Information

 Contains sufficient reagents
for <n> tests

 Temperature Limitation

 Use By/Expiration Date

 CE Symbol

 Caution, consult
accompanying documents

IBD-SCAN®

INTENDED USE

The *IBD-SCAN*® test is a quantitative ELISA for measuring concentrations of fecal lactoferrin, a marker for fecal leukocytes. An elevated level is an indicator of intestinal inflammation. The test can be used as an *in vitro* diagnostic aid to distinguish patients with active inflammatory bowel disease (IBD) from those with noninflammatory irritable bowel syndrome (IBS).

FOR IN VITRO DIAGNOSTIC USE

EXPLANATION

Inflammatory bowel disease (IBD) affects an estimated 1 to 2 million people in the United States (1). Ulcerative colitis and Crohn's disease are the primary subgroups of IBD and both involve chronic inflammation of a noninfectious etiology. In cases of chronic intestinal illnesses, infectious diarrhea that may involve intestinal inflammation must be ruled out to confirm a diagnosis of IBD (e.g., those caused by *Shigella*, *Campylobacter*, and *Clostridium difficile*) (9). Although ulcerative colitis and Crohn's disease differ including disease location and complications, both involve disease states that oscillate between flare and remission. During active disease, leukocytes infiltrate the intestinal mucosa and increase the level of fecal lactoferrin (2-10). IBD patients with active disease may present with symptoms similar to another chronic illness, irritable bowel syndrome (IBS), a noninflammatory condition that may affect as many as 20 million Americans, making it difficult to diagnose in the early stages of disease (1). In persons with IBS, the intestine appears normal upon endoscopic examination, leukocytes are not present in the mucosa, and fecal lactoferrin levels are at baseline (6). In suspected cases of ulcerative colitis and Crohn's disease, colonoscopy and barium x-ray examinations are the most commonly used techniques for confirmation of intestinal inflammation and ulceration (2). A non-invasive quantitative test such as the *IBD-SCAN*® test demonstrates active intestinal inflammation and provides physicians an aid for distinguishing IBS from IBD.

PRINCIPLE OF THE TEST

The *IBD-SCAN*® test uses antibodies to human lactoferrin. The microassay wells supplied with the kit contain immobilized polyclonal antibody against lactoferrin. The detecting antibody consists of polyclonal antibody conjugated to horseradish peroxidase. In the assay, standards and serial dilutions of fecal specimens are transferred to the microassay wells. If detectable levels of lactoferrin are present in the specimen, the lactoferrin will bind to the immobilized antibody. After incubation, the wells are washed and the antibody conjugate is added. The conjugate will bind to the lactoferrin bound during the first incubation phase. Any unbound material is removed during a second series of wash steps. Following the addition of substrate, a color is detected due to the enzyme-antibody-antigen complexes that form in the presence of lactoferrin. The absorbance measured is directly proportional to the concentration of lactoferrin present. Lactoferrin standards ranging from 6.25 to 100 ng/mL are used to generate a standard curve. By plotting absorbance values versus lactoferrin concentrations, the lactoferrin concentration in a test sample can be determined.

DIL 10X

10X Diluent, 40 mL (10X concentrate of a buffered protein solution containing 0.2% thimerosal). The 1X *Diluent* is also used as the negative control (see TEST PROCEDURE)

CONJ ENZ

Conjugate, 7 mL (rabbit polyclonal antibody specific for human lactoferrin conjugated to horseradish peroxidase and in a buffered protein solution containing 0.02% thimerosal)

SUBS REAG

Substrate, 14 mL (solution containing tetramethylbenzidine substrate and peroxide)

LS1-5

Standards, 1.5 mL each of LS1 (100 ng/mL), LS2 (50 ng/mL), LS3 (25 ng/mL), LS4 (12.5 ng/mL), and LS5 (6.25 ng/mL) - human lactoferrin standards in a buffered protein solution containing 0.02% thimerosal

CONTROL +

Positive Control, 1.5 mL (10 µg/mL; human lactoferrin in protein buffered solution containing 0.02% thimerosal)

WASHBUF 20X

Wash Buffer Concentrate, 50 mL (20X concentrate containing phosphate-buffered saline, detergent and 0.2% thimerosal)

H₂SO₄ 0.6N

Stop Solution, 7 mL (0.6 N sulfuric acid). CAUTION: Avoid contact with skin. Flush with water immediately if contact occurs.

MA PLT

Microassay Plate, 12 strips, 8 wells per strip, coated with purified polyclonal antibody specific for lactoferrin (stored with desiccant)

PRECAUTIONS

1. Reagents from different kits should not be mixed. Do not use the kit past the expiration date.
2. Reagents should be removed from the kit box and allowed to reach room temperature before use.
3. Caps and tips are color coded; do not mix!
4. Gently mix all reagents before dispensing.
5. When handling the microassay wells, avoid scratching the bottom of the wells because this may result in elevated absorbance readings.
6. Hold dropper bottles vertically to ensure proper drop size.
7. Handle specimens and used microassay wells as if capable of transmitting infectious agents. Wear gloves when doing the test.
8. Some reagents contain 0.2% thimerosal as a preservative and should be handled with normal laboratory caution.
9. The *Stop Solution* contains 0.6 N sulfuric acid. Flush with water immediately if contact occurs.
10. Unused microassay wells must be placed inside the resealable foil pouch with the desiccant to protect them from moisture.
11. Perform the washing procedure as directed to avoid high background reactions.
12. Use fecal specimens within 2 weeks of collection for optimal results. Frozen specimens (-20°C or lower) may lose activity due to freezing and thawing multiple times.
13. Carefully measure fecal specimens to ensure a correct dilution. Difficult to measure specimens should be weighed.
14. Do not freeze the reagents. Store the kit between 2° and 8°C.
15. The *Substrate* is light sensitive and should be protected from direct sunlight or UV sources.
16. Optimal results are obtained by following the specified test procedure. The concentrations, incubation conditions, and processing specifications have been optimized for sensitivity and specificity. Alterations of the specified procedure and/or test conditions may affect the sensitivity and specificity of the test.
17. The *Positive Control* and *Standards* (LS1-5) contain lactoferrin which is a human derived material. Material has been tested and found negative for antibodies to HIV-1, HIV-2, HCV, and HbsAg. No known test method can offer complete assurance that infectious agents are absent. All human source products should be handled as potentially infectious material. A procedure for handling biohazards is published in the CDC/NIH *Manual of Biosafety in Microbiology & Biomedical Laboratories*.

PRELIMINARY PREPARATIONS

1. Remove all reagents from the kit box to warm to room temperature before use.
2. **Prepare 1X Wash Solution.** The *Wash Solution* is supplied as a 20X concentrate (a precipitate may be noticed). It should be mixed and diluted to a total volume of 1 liter by adding 50 mL of the concentrate to 950 mL of deionized water. Label the bottle. Store any unused 1X *Wash Solution* between 2° and 8°C.

TEST PROCEDURE

Materials provided

2 Plastic adhesive sheets

100 transfer pipettes

Materials and equipment required but not provided

Squirt bottle for 1X *Wash Solution*

Vortex mixer

Refrigerator for storage

Tubes for dilution of specimen

Discard container/absorbent paper

Bottle for 1X *Diluent*

Distilled or deionized water

Incubator set at $37^{\circ}\text{C} \pm 2^{\circ}\text{C}$

ELISA reader (450 nm or 450/620 nm)

- Designate and use 2 wells for each *Standard*, 1 well for the negative control (1X *Diluent*), 1 well for the 1:200 dilution of *Positive Control* and 1 well for specimen dilutions 1:100 and 1:1000. See the table under QUALITY CONTROL for example of well locations.
- Using a calibrated pipette, add 100 μL of each *Standard* LS1-LS5 to duplicate wells and 100 μL of the 1X *Diluent* and *Positive Control* to designated wells.
- Add 100 μL from each specimen dilution (1:100 and 1:1000) to separate wells.
- Cut the adhesive plastic sheet to the size necessary to cover the wells. Cover the wells and incubate them at $37^{\circ}\text{C} \pm 2^{\circ}\text{C}$ for 30 minutes stationary.
- Shake out the contents of the assay wells into a discard pan.
- Wash each well 5 times using the 1X *Wash Solution* in a squirt bottle with a fine tipped nozzle, directing the *Wash Solution* to the bottom of the well with force (i.e. fill the wells, then shake the *Wash Solution* out of the wells into a discard pan). Slap the inverted plate on a dry paper towel and repeat **four times** using a dry paper towel each time. If any particulate matter is seen in the wells, continue washing until all the matter is removed.
- Add 1 drop of *Conjugate* (red cap) to each well. Incubate the wells at $37^{\circ}\text{C} \pm 2^{\circ}\text{C}$ for 30 minutes stationary.
- Repeat step #6. *Dispose of paper towels and specimen containers properly.*
- Add 2 drops of *Substrate* (blue cap) to each well. Gently tap the wells to mix the contents. Incubate the wells at room temperature for 15 minutes. Gently tap the wells 1 or 2 times during this incubation period.
- Add 1 drop of *Stop Solution* (yellow cap) to each well. Gently tap the wells to mix and wait 2 minutes before reading. The addition of the *Stop Solution* converts the blue color to a yellow color which may be quantitated by measuring the optical density at 450 nm or 450/620 nm on a microplate ELISA reader. Wipe the underside of each well with a soft paper towel before measuring the optical density. Read within two to ten minutes after adding *Stop Solution*.
- Record absorbance values for the positive control dilution, for the negative control, for each specimen dilution, and for the standards.
- Average the acceptable readings of duplicate wells before interpreting results.

QUALITY CONTROL


The negative control well containing 1X *Diluent* should have an $\text{OD}_{450} < 0.100$ or $\text{OD}_{450/620} < 0.060$. The calculated concentration for the *Positive Control* should be in the range of $10 \pm 3 \mu\text{g/mL}$ recovery. Typical layout and values for the standards and samples are shown in the following table and graph. Following the Linear Trend/Regression Type analysis, the R^2 value should be ≥ 0.98 . If graph paper is used, points should appear in a straight line.

Typical Layout for Test Samples

LS1 - LS5 - Lactoferrin standards S1 - S18 - Specimens at 1/100 and 1/1000 dilutions

	1	2	3	4	5	6
A	NC	PC(200)	S3(100)	S3(1000)	S11(100)	S11(1000)
B	LS1	LS1	S4(100)	S4(1000)	S12(100)	S12(1000)
C	LS2	LS2	S5(100)	S5(1000)	S13(100)	S13(1000)
D	LS3	LS3	S6(100)	S6(1000)	S14(100)	S14(1000)
E	LS4	LS4	S7(100)	S7(1000)	S15(100)	S15(1000)
F	LS5	LS5	S8(100)	S8(1000)	S16(100)	S16(1000)
G	S1(100)	S1(1000)	S9(100)	S9(1000)	S17(100)	S17(1000)
H	S2(100)	S2(1000)	S10(100)	S10(1000)	S18(100)	S18(1000)

Typical Absorbance Values (OD₄₅₀) for the Lactoferrin Standard Curve

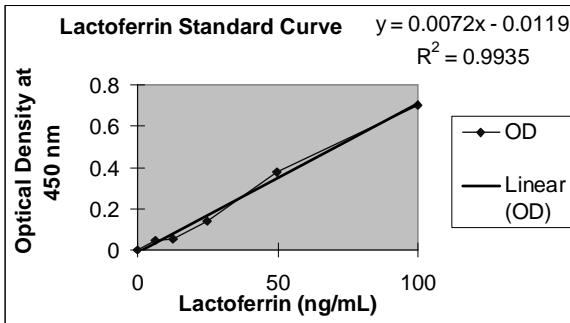

CALCULATION OF RESULTS

The results in this insert were determined using a Linear Trend/Regression Type analysis. Other data reduction methods may give slightly different results.

1. An appropriate data reduction computer program, using Linear Trend/Regression Type analysis, should be used for optimal estimation of sample values. If a computer program is not available, the data may be plotted using graph paper.
2. Choose the most diluted specimen that gives an OD₄₅₀ or OD_{450/620} value within the standard curve and OD ≥ 0.100 or 0.060 , respectively. If both sample dilutions have absorbance readings greater than the highest concentration of standard, repeat using additional 1:10 dilutions. Conversely, any sample having an absorbance reading less than the lowest concentration of standard should be retested using the 1:10 dilution and if found negative recorded as $<1 \mu\text{g/g}$ wet weight.
3. Plot the average absorbance values of the *Standards* on the y-axis versus the concentration on the x-axis.
4. Perform the Linear Trend/Regression Type analysis and determine if the R^2 value is ≥ 0.98 .
5. Instruct the program to produce the equation for the plotted line. The equation should fit the equation of a line which is $Y = MX + B$, where $Y = \text{OD}_{450}$ or $\text{OD}_{450/620}$ of the sample, $M = \text{Slope}$, $B = \text{Y-intercept}$ and $X = \text{Concentration of the unknown sample}$.
6. Solve the equation for X to determine the concentration of lactoferrin in the specimen.
7. Multiply the value of the unknown sample by the dilution factor.
8. Divide by 1000 to convert ng/mL to $\mu\text{g/mL}$ (approximately $\mu\text{g/g}$ wet weight).

Example Calculation

1. A graph was produced using the data provided in the Quality Control section of this Package Insert.
2. Linear analysis of the graph produced the following equation: $y = 0.0072x - 0.0119$ and an R^2 value of 0.99.
3. The 1:1000 dilution of specimen #2 was picked for analysis with an absorbance value of 0.450.
4. Solving for X yields: $X = 64$ ng/mL.
5. Multiply by the dilution factor: $64 \times 1000 = 64,000$ ng/mL.
6. Convert to $\mu\text{g/g}$ by dividing by 1000: $64,000 / 1000 = 64$ $\mu\text{g/g}$ wet weight.

INTERPRETATION OF VALUES

Lactoferrin Level in feces	Interpretation of results
0 to 7.24 $\mu\text{g/mL}$ (g) feces	Baseline (normal)
≥ 7.25 $\mu\text{g/mL}$ (g) feces	Elevated

SHELF-LIFE AND STORAGE

The expiration date is given on the outside label of the kit. Expiration dates for each component are listed on the individual labels. The kit containing the reagents with designated shelf-life should be stored between 2° and 8°C and should be returned to the refrigerator as soon as possible after use.

PERFORMANCE CHARACTERISTICS

A multi-center clinical study (3 sites) was done evaluating fecal lactoferrin levels in 180 patients suffering with IBS and IBD (ulcerative colitis disease and Crohn's disease), and compared to 56 healthy persons. Patients were assessed for active disease using the Harvey Bradshaw Activity Index (HBAI) and fecal samples were collected for lactoferrin analysis. Patients with IBS had lactoferrin levels similar to healthy control persons ($p > 0.999$). Fecal lactoferrin levels were significantly greater in patients with Crohn's disease and ulcerative colitis, compared to healthy controls ($p < 0.05$, $p < 0.0006$). A significant number of patients defined as inactive using HBAI had elevated fecal lactoferrin indicating intestinal inflammation. Fecal lactoferrin levels for the study population and statistical analysis of *IBD-SCAN*[®] test results as compared to the HBAI are shown in Table 1 and Table 2, respectively.

Table 1. Fecal lactoferrin levels of the study population

Study Population N=235	No. of specimens	Fecal lactoferrin (mean $\mu\text{g/mL} \pm \text{SE}$)
Inactive UC	41	65.65 \pm 24.20
Active UC	31	1814.89 \pm 788.25
Inactive CD	26	239.41 \pm 82.73
Active CD	51	672.11 \pm 241.79
IBS	31	1.27 \pm 0.29
Healthy persons	55	1.55 \pm 0.41

Table 2. *IBD-SCAN*[®] test results for distinguishing active inflammatory bowel disease from irritable bowel syndrome/healthy persons

N=178	Active IBD based on HBAI assessment ≥ 4	IBS (31) /Healthy Persons (55) based on clinical and self assessment
<i>IBD-SCAN</i> [®] test Elevated	75	3
<i>IBD-SCAN</i> [®] test Baseline	17	83

Sensitivity	81.5%
Specificity	96.5%
Predictive Positive Value	96.2%
Predictive Negative Value	83.0%
Correlation	88.8%

LIMITATIONS OF THE PROCEDURE

1. The *IBD-SCAN*[®] test is a quantitative test that measures the level of fecal lactoferrin released from leukocytes. The test may not be appropriate in immunocompromised persons. The following patient samples should be excluded from use in the *IBD-SCAN*[®] test: patients with a history of HIV and/or Hepatitis B and C, patients with a history of infectious diarrhea (within 6 months), and patients having had a colostomy and/or ileostomy within 1 month.
2. Fecal lactoferrin concentrations should not be interpreted as absolute evidence for the presence of a gastrointestinal illness. Prediction of active and inactive disease should be based on a complete clinical evaluation of the patient that may also include multiple fecal lactoferrin level determinations.
3. At this time, the *IBD-SCAN*[®] test has not been clinically evaluated for use in the detection of leukocytes in other types of clinical specimens. It should be used only for the analysis of fecal specimens.
4. Fecal specimens that have been preserved in 10% Formalin, Merthiolate Formalin, Sodium Acetate Formalin, or Polyvinyl Alcohol cannot be used.
5. Other intestinal ailments, including many gastrointestinal infections and colorectal cancer, often result in elevated levels of lactoferrin in fecal specimens. Therefore, when evaluating a patient, a clinical assessment must be considered along with *IBD-SCAN*[®] test results.
6. High levels of fecal lactoferrin may be observed with clinical specimens. Specimens should be serially diluted until the absorbance value falls within the lactoferrin standard curve.

CROSS-REACTIVITY

Various intestinal organisms were examined for cross-reactivity in the *IBD-SCAN*[®] test. For the analysis, broth cultures mixed with 1X *Diluent* were evaluated. Broth cultures at log phase containing $\geq 10^8$ bacteria per mL were used. Organisms that did not react in the *IBD-SCAN*[®] test are listed as follows:

<i>Acinetobacter Iwoffii</i>	<i>Clostridium novyi</i> (types A,B,C)
<i>Aeromonas hydrophila</i>	<i>Clostridium perfringens</i> (types A,B,C,D,E)
<i>Bacillus cereus</i>	<i>Clostridium septicum</i>
<i>Bacillus subtilis</i>	<i>Clostridium sporogenes</i>
<i>Bacteroides distasonis</i>	<i>Clostridium tetani</i>
<i>Bacteroides eggerthii</i>	<i>Enterococcus faecalis</i>

<i>Bacteroides fragilis</i>	<i>Eubacterium aerofaciens</i>
<i>Bacteroides ovatus</i>	<i>Escherichia coli</i>
<i>Bacteroides stercoris</i>	<i>Fusobacterium prausnitzii</i>
<i>Bacteroides thetaiotaomicron</i>	<i>Klebsiella pneumoniae</i>
<i>Bacteroides uniformis</i>	<i>Peptostreptococcus anaerobius</i>
<i>Bacteroides vulgatus</i>	<i>Proteus vulgaris</i>
<i>Bifidobacterium adolescentis</i>	<i>Pseudomonas aeruginosa</i>
<i>Bifidobacterium longum</i>	<i>Salmonella choleraesuis</i>
<i>Campylobacter jejuni</i>	<i>Salmonella enteritidis</i>
<i>Candida albicans</i>	<i>Salmonella typhi</i>
<i>Candida krusei</i>	<i>Salmonella typhimurium</i>
<i>Candida tropicalis</i>	<i>Shigella dysenteriae</i>
<i>Clostridium bifermentans</i>	<i>Shigella flexneri</i>
<i>Clostridium chauvoei</i>	<i>Shigella sonnei</i>
<i>Clostridium difficile</i>	<i>Staphylococcus aureus</i>
<i>Clostridium haemolyticum</i>	<i>Vibrio parahaemolyticus</i>
<i>Clostridium histolyticum</i>	<i>Yersinia enterocolitica</i>

EFFECT OF FECAL SAMPLE CONSISTENCY

There were no differences observed between fecal specimens having liquid, semi-solid, or solid consistency when compared to the *IBD-CHEK*[®] test results and/or clinical assessments for disease activity.

REPRODUCIBILITY AND PRECISION

The inter-assay variation was determined by quantitatively analyzing 9 fecal specimens over a 3 day period. The %CV ranged from 12.0% to 47.7%, with a mean value of 33.5% for positive specimens. The intra-assay variation was determined by quantitatively analyzing 9 fecal specimens using 4 replicates in one lot of kits. The %CV ranged from 7.9% to 16.0%, with a mean value of 12.0% for positive specimens.

REFERENCES

1. Everhart, J. E. 1994. Digestive Diseases in the United States: Epidemiology and Impact. U.S. Department of Health and Human Services, National Institutes of Health, National Institute of Diabetes and Digestive and Kidney Diseases. U.S. Government Printing Office, NIH Publication no. 94-1447.
2. Fine., K.D., F. Ogunji, J. George, M. Niehaus, and R.L. Guerrant. 1998. Utility of a rapid fecal latex agglutination test detecting the neutrophil protein lactoferrin, for diagnosing inflammatory causes of chronic diarrhea. *Am. J. Gastroenterol.* 93:1300-1305.
3. Guerrant, R.L., V. Araujo, E. Soares, K. Kotloff, A. Lima, W. Cooper, and A. Lee. 1992. Measurement of fecal lactoferrin as a marker of fecal leukocytes. *J. Clin. Microbiol.* 30:1238-1242.
4. Harris, J. C., H. L. DuPont, and B. R. Hornick. 1971. Fecal leukocytes in diarrheal illness. *Ann. Intern. Med.* 76:697-703.
5. Huicho L., V. Garaycochea, N. Uchima, R. Zerpa, and R.L. Guerrant. 1997. Fecal lactoferrin, fecal leukocytes and occult blood in the diagnostic approach to childhood invasive diarrhea. *Pediatr. Infect. Dis. J.* 16(7):644-647.
6. Kane, S., W. Sandborn, P. Rufo, A. Zholudev, J. Boone, D. Lyerly, M. Camilleri, and S. Hanauer. 2003. Fecal lactoferrin is a sensitive and specific marker in identifying intestinal inflammation. *Am. J. Gastroenterol.* 98:1309-1314.
7. Kayazawa, M., O. Saitoh, K. Kojima, K. Nakagawa, S. Tanaka, K. Tabata, R. Maysuse, K. Uchida, M. Hoshimoto, I. Hirata, and K. Katsu. 2002. Lactoferrin in whole gut lavage fluid as a marker for disease activity in inflammatory bowel disease: Comparison with other neutrophil-derived proteins. *Am. J. Gastroenterol.* 97:360-369.
8. Parsi, M., B. Shen, J. Achkar, F. Remzi, J. Goldblum, J. Boone, D. Lin, J. Connor, V. Fazio, and B. Lashner. 2004. Fecal lactoferrin for the diagnosis of symptomatic patients with ileal pouch-anal anastomosis. *Gastroenterology* 126:1280-1286.
9. Sartor, R. B. 1995. Microbial agents in pathogenesis, differential diagnosis, and complications of inflammatory bowel disease. In M. Blaser, P. Smith, J. Ravdin, H. Greenberg, and R. Guerrant (ed.), *Infections of the Gastrointestinal Tract*. Raven Press, New York, NY.
10. Sugi, K., O. I. Saitoh, and K. Katsu. 1996. Fecal lactoferrin as a marker for disease activity in inflammatory bowel disease: Comparison with other neutrophil-derived proteins. *Am. J. Gastroenterol.* 91:927-934.